



**SCREEN 1 BENZODIAZEPINE
(Urine)
Package Insert**

REF: SC-0036-25 English

A rapid test for the qualitative detection of Benzodiazepines in human urine.
For medical and other professional in vitro diagnostic use only.

INTENDED USE

The BZO Rapid Test Panel (Urine) is a rapid chromatographic immunoassay for the detection of Oxazepam (major metabolite) in urine at a cut-off concentration of 300ng/ml. This test will detect other related compounds, please refer to the Analytical Specificity table in this package insert.

This assay provides only a qualitative, preliminary analytical test result. A more specific alternate chemical method must be used in order to obtain a confirmed analytical result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method. Clinical consideration and professional judgment should be applied to any drug of abuse test result, particularly when preliminary positive results are used.

SUMMARY

Benzodiazepines are medications that are frequently prescribed for the symptomatic treatment of anxiety and sleep disorders. They produce their effects via specific receptors involving a neurochemical called gamma aminobutyric acid (GABA). Because they are safer and more effective, Benzodiazepines have replaced Barbiturates in the treatment of both anxiety and insomnia. Benzodiazepines are also used as sedatives before some surgical and medical procedures, and for the treatment of seizure disorders and alcohol withdrawal.

Risk of physical dependence increases if Benzodiazepines are taken regularly (e.g., daily) for more than a few months, especially at higher than normal doses. Stopping abruptly can bring on such symptoms as trouble sleeping, gastrointestinal upset, feeling unwell, loss of appetite, sweating, trembling, weakness, anxiety and changes in perception. Only trace amounts (less than 1%) of most Benzodiazepines are excreted unaltered in the urine; most of the concentration in urine is conjugated drug. The detection period for the Benzodiazepines in the urine is 3-7 days.

The BZO Rapid Test Panel (Urine) is a rapid urine-screening test that can be performed without the use of an instrument. The test utilizes the antibody to selectively detect elevated levels of Benzodiazepines in urine. The BZO Benzodiazepines Test Panel (Urine) yields a positive result when the Benzodiazepines in urine exceeds the cut-off level.

PRINCIPLE

The BZO Rapid Test Panel (Urine) is an immunoassay based on the principle of competitive binding. Drugs which may be present in the urine specimen compete against the drug conjugate for binding sites on the antibody.

During testing, a urine specimen migrates upward by capillary action. Benzodiazepines, if present in the urine specimen below the cut-off level, will not saturate the binding sites of the antibody in the test. The antibody coated particles will then be captured by immobilized Benzodiazepines-protein conjugate and a visible colored line will show up in the test line region. The colored line will not form in the test line region if the Benzodiazepines level exceeds the cut-off level, because it will saturate all the binding sites of anti-Benzodiazepines antibody.

A drug-positive urine specimen will not generate a colored line in the test line region because of drug competition, while a drug-negative urine specimen or a specimen containing a drug concentration less than the cut-off will generate a line in the test line region. To serve as a procedural control, a colored line will always appear at the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

REAGENTS

The test contains mouse monoclonal anti-Benzodiazepines antibody coupled particles and Benzodiazepines-protein conjugate. A goat antibody is employed in the control line system.

PRECAUTIONS

- For medical and other professional in vitro diagnostic use only. Do not use after the expiration date.
- The test should remain in the sealed pouch until use.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used test should be discarded according to local regulations.

STORAGE AND STABILITY

Store as packaged at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use beyond the expiration date.

SPECIMEN COLLECTION AND PREPARATION

Urine Assay

The urine specimen must be collected in a clean and dry container. Urine collected at any time of the day may be used. Urine specimens exhibiting visible particles should be centrifuged, filtered, or allowed to settle to obtain a clear specimen for testing.

Specimen Storage

Urine specimens may be stored at 2-8°C for up to 48 hours prior to testing. For prolonged storage, specimens may be frozen and stored below -20°C. Frozen specimens should be thawed and mixed before testing.

MATERIALS


Materials Provided

- Test Panels
- Package insert
- Materials Required But Not Provided**
- Specimen collection container
- Timer

DIRECTIONS FOR USE

Allow test, urine specimen, and/or controls to reach room temperature (15-30°C) prior to testing.

1. Bring the pouch to room temperature before opening it. Remove the test panel from the sealed pouch and use it within one hour.
2. Remove the cap.
3. With the arrow pointing toward the urine specimen, immerse the test panel vertically in the urine specimen for at least 10 to 15 seconds. Immerse the strip to at least the level of the wavy lines, but not above the arrow on the test panel.
4. Replace the cap and place the test panel on a non-absorbent flat surface.
5. Start the timer and wait for the colored line(s) to appear.
6. **The result should be read at 5 minutes.** Do not interpret the result after 10 minutes.

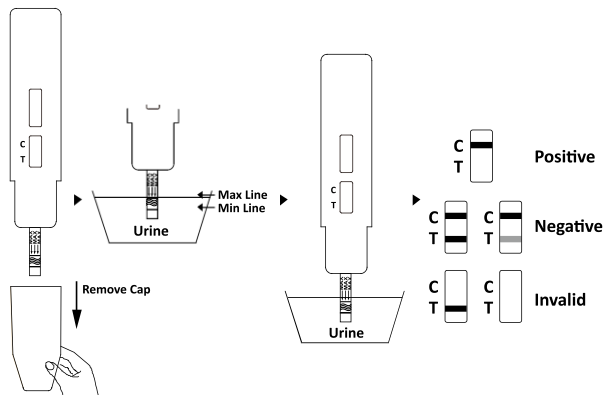

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

NEGATIVE:* Two colored lines appear. One colored line should be in the control line region (C), and another apparent colored line should be in the test line region (T). This negative result indicates that the Benzodiazepine concentration is below the detectable cut-off level.

***NOTE:** The shade of color in the test line region (T) may vary, but it should be considered negative whenever there is even a faint colored line.

POSITIVE: One colored line appears in the control line region (C). No line appears in the test line region (T). This positive result indicates that the Benzodiazepine concentration exceeds the detectable cut-off level.

INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

QUALITY CONTROL

A procedural control is included in the test. A colored line appearing in the control line region (C) is considered an internal procedural control. It confirms sufficient specimen volume, adequate membrane wicking and correct procedural technique. Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as good laboratory testing practice to confirm the test procedure and to verify proper test performance.

LIMITATIONS

1. The BZO Rapid Test Panel (Urine) provides only a qualitative, preliminary analytical result. A secondary analytical method must be used to obtain a confirmed result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method.1,2
2. It is possible that technical or procedural errors, as well as other interfering substances in the urine specimen may cause erroneous results.
3. Adulterants, such as bleach and/or alum, in urine specimens may produce erroneous results regardless of the analytical method used. If adulteration is suspected, the test should be repeated with another urine specimen.
4. A positive result indicates presence of the drug or its metabolites but does not indicate level of intoxication, administration route or concentration in urine.
5. A negative result may not necessarily indicate drug-free urine. Negative results can be obtained when drug is present but below the cut-off level of the test.
6. Test does not distinguish between drugs of abuse and certain medications.

EXPECTED VALUES

This negative result indicates that the Benzodiazepines concentration is below the detectable level of 300ng/ml. Positive result means the concentration of Benzodiazepines is above the level of 300ng/ml. The BZO Rapid Test Panel has a sensitivity of 300ng/ml.

PERFORMANCES CHARACTERISTICS

Accuracy

A side-by-side comparison was conducted using The BZO Rapid Test Panel (Urine) and a commercially available BZO rapid test. Testing was performed on 95 clinical specimens previously collected from subjects present for Drug Screen Testing. The following results were tabulated:

BZO Rapid Test Panel	Method	Other BZO Rapid Test		Total Results
	Results	Positive	Negative	
	Positive	43	0	43
	Negative	0	52	52
Total Results		43	52	95
% Agreement		>99.9%	>99.9%	>99.9%

A side-by-side comparison was conducted using The BZO Rapid Test Panel (Urine) and GC/MS at the cut-off of 300ng/ml. Testing was performed on 250 clinical specimens previously collected from subjects present for Drug Screen Testing. The following results were tabulated:

Method		GC/MS		Total Results
BZO Rapid Test Panel	Results	Positive	Negative	122
	Positive	121	1	
	Negative	2	126	
Total Results		123	127	250
% Agreement		98.4%	99.2%	98.8%

Analytical Sensitivity

A drug-free urine pool was spiked with Oxazepam at the following concentrations: 0ng/ml, 150ng/ml, 225 ng/ml, 300ng/ml, 375ng/ml, 450ng/ml and 900 ng/ml. The result demonstrates >99% accuracy at 50% above and 50% below the cut-off concentration. The data are summarized below:

Oxazepam Concentration (ng/mL)	Percent of Cut-off	n	Visual Result	
			Negative	Positive
0	0	30	30	0
150	-50%	30	30	0
225	-25%	30	27	3
300	Cut-off	30	15	15
375	+25%	30	3	27
450	+50%	30	0	30
900	3X	30	0	30

Analytical Specificity

The following table lists compounds that are positively detected in urine by the BZO Rapid Test Panel (Urine) at 5 minutes.

Compound	Concentration (ng/mL)	Compound	Concentration (ng/mL)
Alprazolam	100	Flunitrazepam	200
a-hydroxyalprazolam	1,500	(±) Lorazepam	3,000
Bromazepam	900	RS-Lorazepam	200
Chlordiazepoxide	900	Midazolam	6,000
Clobazam	200	Nitrazepam	200
Clonazepam	500	Norchlordiazepoxide	100
Clorazepate	500	Nordiazepam	900
Delorazepam	900	Oxazepam	300
Desalkylflurazepam	200	Temazepam	100
Diazepam	300	Triazolam	3,000
Estazolam	6,000		

Precision

A study was conducted at three hospitals by laypersons using three different lots of product to demonstrate the within run, between run and between operator precision. An identical panel of coded specimens containing, according to GC/MS, no Oxazepam, 25% Oxazepam above and below the cut-off and 50% Oxazepam above and below the 300ng/ml cut-off was provided to each site. The following results were tabulated:

Oxazepam Concentration (ng/mL)	n per Site	Site A		Site B		Site C	
		-	+	-	+	-	+
0	10	10	0	10	0	10	0
150	10	10	0	10	0	10	0
225	10	9	1	9	1	9	1
375	10	1	9	1	9	1	9
450	10	0	10	0	10	0	10

Effect of Urinary Specific Gravity

Fifteen urine specimens of normal, high, and low specific gravity ranges were spiked with 150ng/ml and 450ng/ml of Oxazepam. The BZO Test Panel (Urine) was tested in duplicate using the fifteen neat and spiked urine specimens. The results demonstrate that varying ranges of urinary specific gravity do not affect the test results.

Effect of Urinary pH

The pH of an aliquoted negative urine pool was adjusted to a pH range of 5 to 9 in 1 pH unit increments and spiked with Oxazepam to 150ng/ml and 450ng/ml. The spiked, pH-adjusted urine was tested with the BZO Rapid Test Panel (Urine) in duplicate. The results demonstrate that varying ranges of pH do not interfere with the performance of the test.

Cross-Reactivity

A study was conducted to determine the cross-reactivity of the test with compounds in either drug-free urine or Oxazepam positive urine. The following compounds show no cross-reactivity when tested with the BZO Rapid Test Panel (Urine) at a concentration of 100 µg/ml.

Non Cross-Reacting Compounds

Acetaminophen	Deoxycorticosterone	MDE	β-Phenylethylamine
Acetophenetidin	Dextromethorphan	Meperidine	Phenylpropanolamine
N-Acetylprocainamide	Diclofenac	Meprobamate	Prednisolone
Acetylsalicylic acid	Diflunisal	Methadone	Prednisone
Aminopyrine	Digoxin	L-Methamphetamine	Procaine
Amitypyline	Diphenhydramine	Methoxyphenamine	Promazine
Amobarbital	Doxylamine	(±) - 3,4-Methylenedioxy-amphetamine	Promethazine
Amoxicillin	Ecgonine	(±) - 3,4-Methylenedioxy-methamphetamine	D,L-Propranolol
Ampicillin	Ecgonine methylester	Morphine-3-β-D-glucuronide	D-Propoxyphene
L-Ascorbic acid	(-)-ψ-Ephedrine	Morphine Sulfate	D-Pseudoephedrine
D,L-Amphetamine sulfate	[1R,2S] (-) Ephedrine sulfate	Nalidixic acid	Quinacrine
Apomorphine	(L) - Epinephrine	Naloxone	Quinidine
Aspartame	Erythromycin	Naltrexone	Quinine
Atropine	β-Estradiol	Naproxen	Ranitidine
Benzilic acid	Estrone-3-sulfate	Niacinamide	Salicylic acid
Benzoic acid	Ethyl-p-aminobenzoate	Nifedipine	Secobarbital
Benzoyllecgonine	Fenopropfen	Norcocodein	Serotonin
Benzphetamine	Furosemide	Norethindrone	Sulfamethazine
Bilirubin	Gentisic acid	D-Norpropoxyphene	Sulindac
(±) - Brompheniramine	Hemoglobin	Noscapine	Tetracycline
Caffeine	Hydralazine	D,L-Octopamine	Tetrahydrocortisone, 3-Acetate
Cannabidiol	Hydrochlorothiazide	Oxalic acid	Tetrahydrocortisone 3-(β-D-glucuronide)
Cannabinol	Hydrocodone	Oxolinic acid	Tetrahydrozoline
Chloralhydrate	Hydrocortisone	Oxycodone	Thiamine
Chloramphenicol	O-Hydroxyhippuric acid	Oxymetazoline	Thioridazine
Chlorothiazide	p-Hydroxyamphetamine	Papaverine	D,L-Tyrosine
(±) - Chlorpheniramine	p-Hydroxy-methamphetamine	Penicillin-G	Tolbutamide
Chlorpromazine	3-Hydroxytyramine	Pentazocine	Triamterene
Chlorquine	Ibuprofen	Pentobarbital	Trifluoperazine
Cholesterol	Imipramine	Perphenazine	Trimethoprim
Clomipramine	lproniazid	Phencyclidine	Trimipramine
Clonidine	(±) - Isoproterenol	Phenelzine	Tryptamine
Cocaethylene	Isoxsuprine	Phenobarbital	D,L-Tryptophan
Cocaine	Ketamine	Phentermine	Tyramine
Cortisone	Ketoprofen	Trans-2-phenylcyclopropylamine hydrochloride	Uric acid
(-) Cotinine	Labetalol	L-Phenylephrine	Verapamil
Creatinine	Loperamide		Zomepirac
	Maprotiline		

BIBLIOGRAPHY

- Baselt RC. Disposition of Toxic Drugs and Chemicals in Man. 2nd Ed. Biomedical Publ., Davis, CA. 1982; 488
- Hawks RL, CN Chiang. Urine Testing for Drugs of Abuse. National Institute for Drug Abuse (NIDA), Research Monograph 73, 1986.

INDEX OF SYMBOLS

	Consult Instructions For Use		Tests per kit		Authorized Representative
	For in vitro diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		Catalog #
	Do not use if package is damaged		Manufacturer		



SCREEN ITALIA S.r.l.
Via dell'Artigianato, 16
06089 - Torgiano - Perugia - Italia
www.screenitalia.it info@screenitalia.it



Number: 146174101
Effective Date: 2021-06-10